

LS126C

UV Light Meter

User Manual V2.1



Scan the QR code download and install the App

Please read this manual carefully before using and reserve it for reference.

I. Product introduction


The UVC is also known as short-wave sterilization ultraviolet light. 253.7nm wavelength ultraviolet radiation from low pressure mercury lamp is widely used in ultraviolet sterilization industry. LS126C UV light meter is specially designed to measure UVC intensity and energy values, which is widely applied in hospitals, CDC, pharmaceutical companies, FDA, etc. for UV intensity and energy measurement.

II. Technical Parameters

1. Spectral response: 230nm-280nm, $\lambda_p = 254\text{nm}$
2. Power measuring range: 0 - 20000 $\mu\text{W}/\text{cm}^2$
3. Power resolution: 0.1 $\mu\text{W}/\text{cm}^2$
4. Energy measuring range: 0-9999999 $\mu\text{J}/\text{cm}^2$
5. Relative indication error (H is the standard value): $H < 50 \mu\text{W}/\text{cm}^2$: $\pm 4 \mu\text{W}/\text{cm}^2$, $H \geq 50 \mu\text{W}/\text{cm}^2$: $\pm 8\%H$ (relative to NIM standard)
6. Long wave response error: $< 60\%$
7. Cosine characteristics (directional response) error: 10%
8. Linearity error: $\pm 1\%$
9. Short-term instability: $\pm 1\%$ (30min after startup)
10. Fatigue characteristics: attenuation $< 2\%$
11. Error of zero: $\pm 0.1\%$ of full scale
12. Response time: < 0.5 seconds
13. Power data storage interval: 1s/10s/60s optional
14. Recording period: 10 min / 100 min / 600 min
15. Bluetooth transmission distance: 50 meters (open area)
16. Instrument size: 148mm long * 76mm wide * 26mm high
17. Probe size: diameter 39mm * thickness 15mm
18. Probe wire length: 1 meter
19. Instrument weight: about 300 grams
20. Display: 240*160 dot matrix LCD
21. Battery: 4 AAA alkaline dry batteries
22. Operating Temperature: 0° to 40°C , $< 85\% \text{RH}$

III. Spectral response curve

Use of high-precision UVC optical filters and professional UV sensor allows the instrument to almost give no response to UVA, UVB, visible light, etc.

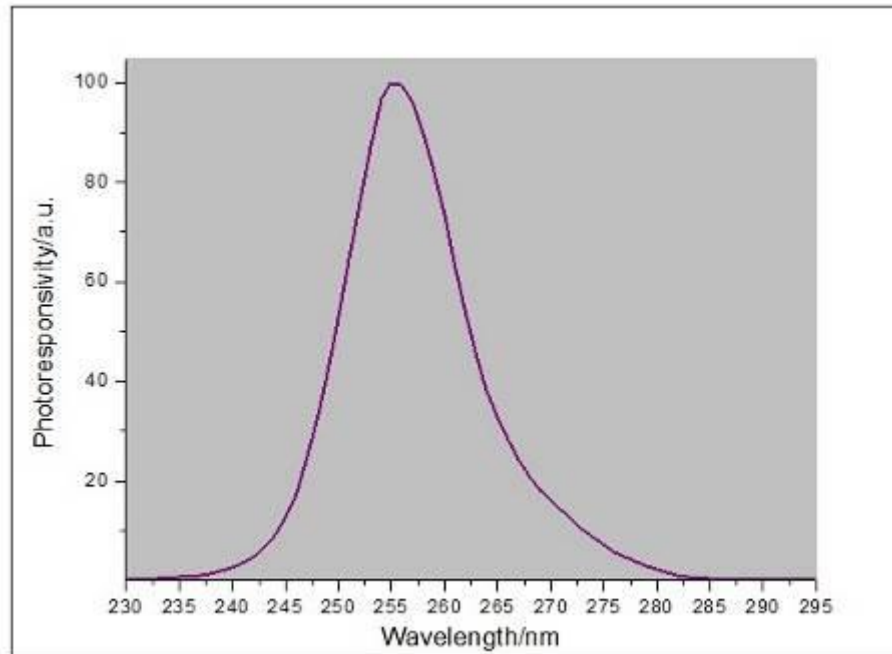


IV. Product features


1. Specially designed for 253.7nm UV germicidal lamps (low-pressure mercury lamps).
2. Self-equipped with Bluetooth, Mobile phone APP can get data from LS126C through Bluetooth Wireless Transmission.
3. Self-equipped with a real-time clock that can be used to trace the accurate time of the measurement result.
4. Data storage automatically before timing shutdown, which makes unattended measurements possible.
5. High-precision UVC optical filters and professional UV sensor, which allow the instrument to almost give no response to other wavebands.
6. Equipped with USB interface and dedicated PC software featured with parameter configuration, data reading, and UV power curve, exporting of UV power data to EXCEL, report generation functions.
7. With power curve display function and statistical function (real-time value, maximum value, minimum value, average value, measurement duration, date/time, Energy value), which is used to analyze the change trend of the luminous intensity after lightening the lamp.


8. Advanced digital probe technology, by which analog signal conversion to digital signal on the probe.

V. Operations


1. Power on/off

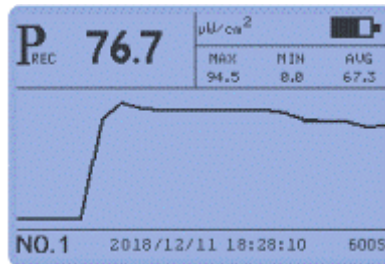


- **Power on:** Press  to power on the instrument. After powering on, the instrument displays the information of the calibration date, production date, version number and serial number. Then, the latest record is displayed, as shown below:




- **Power off:** Long press the  button to power off; or the instrument will automatically power off when "Auto Off" set to ON.
- The data recorded automatically before shutdown, when instrument power on, the latest recorded (No.1 record) displayed.

2. Parameter settings mode

In the off state, long press the  button 3s to enter the parameter setting mode. In the setting mode,

 and  are Select buttons, and  is the confirm button.

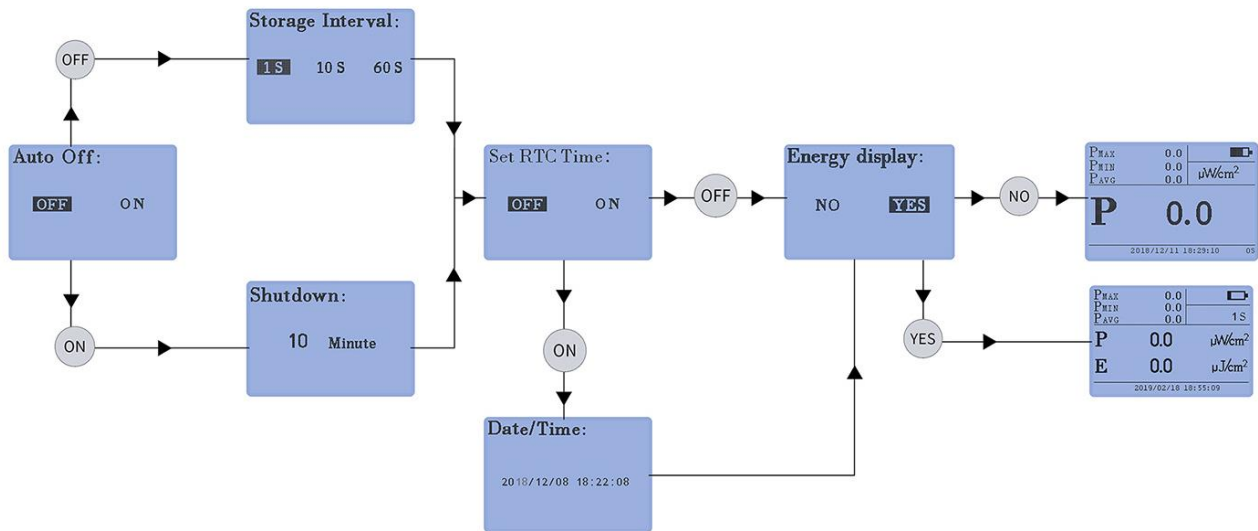

A. Select whether automatically power off or not (Auto Off: ON/OFF)

Short press the “▲” or “▼” button to select ON/OFF

Selecting ON indicates that the instrument automatically powers off as long as no operation within the set time.

Selecting OFF indicates that the user has to manually turn the instrument off, and the instrument will not automatically power off.

If you select ON and press “DEL”, the system will enter “Shutdown” in which Setting automatic shutdown time

If you select OFF and press “DEL”, the system will enter “Storage Interval” in which you can set the storage interval.

B. Setting of automatic shutdown time (Shutdown: 1 minute to 10 minutes)

Short press “▲” or “▼” to set the shutdown time. The system will automatically power off if there is no operation within the set time. When Auto Off set ON, the system stores the data every 1 second and saves the record to the data record of No.1. Short press the “DEL” button to confirm the setting.

C. Storage interval setting (Storage interval: 1s/10s/60s)

When setting Auto Off is off, the instrument stores data according to the storage interval. For each record, there are up to 600 measured values stored. The larger the storage interval is, the longer the recording period will be. The storage interval 1s/10s/60s correspond to the recording period 10 minutes / 100 minutes / 600 minutes, respectively. When the number of the stored value exceeds 600, the oldest measured value is automatically deleted, and the most recent values are kept.

Short press “▲” or “▼” button to set the storage interval, short press “DEL” button to confirm the setting.

D. Set RTC Time: ON/OFF

Short press the “▲” or “▼” button to select ON/OFF

Select ON to set the RTC. Short press the “DEL” button to enter the Date/Time setting.

Select OFF not to set the RTC, Short press “DEL” to enter the next setting: whether to display energy.

E. Setting Date/Time of the RTC

Short press “▲” or “▼” button to progressively increase or decrease the current flashing item; short press “DEL” to make a switch among year, month, day, hour, minute and second. Short press “HOLD” to enter the next setting mode: whether to display energy.

F. Energy Display: NO/YES


Short press “▲” or “▼” button to select NO/YES.







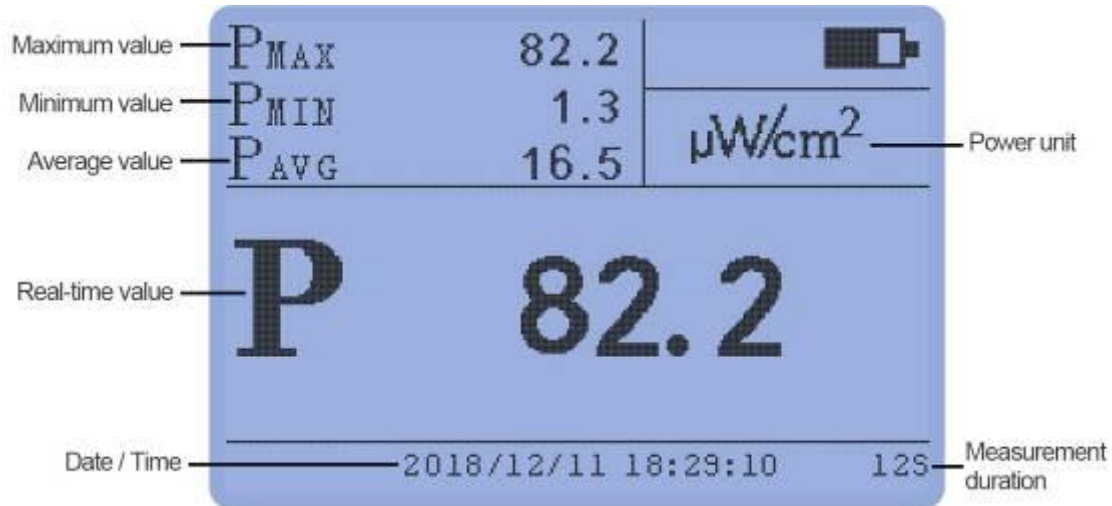

Select YES to display energy, select NO not to display energy.

Short press “DEL” to save and exit the setting mode, the instrument enters the measurement mode.





3. Measurement mode

- In record data query mode, press the “HOLD” button to enter the measurement mode. The system displays the real-time value of the power, maximum value, minimum value, average value, measurement duration, real-time clock and energy values (according to the setting whether to display).



- In the measurement mode, if the backlight is off, press the  button to light the backlight; if the backlight is already lit, short press the  button, and the “HOLD” icon will be displayed in the lower left corner of the interface. All data will be holding on the LCD, and the current data will be recorded.
- In the “HOLD” state, if the backlight is off, press the  button to light the backlight; if the backlight is already lit, short press the  button to cancel the HOLD state and start a new measurement.
- In the measurement mode, if the backlight is off, short press the  button to light the backlight; if the backlight is already lit, press the  button to clear up the current data and start a new measurement.
- In the measurement mode, short press  or  to enter the Record data query mode

4. Record data query mode

- After power on, enter the Record data query mode. The instrument will display the latest recorded data No.1 (up to 25 recorded data are stored in the instrument, and the oldest recorded data will be deleted automatically when exceed 25 recorded data).
- Short press  or  to scroll up or down a recorded data.
- Long press the  button 3S to clear all recorded data.
- Short press the  button to enter the measurement mode.


5. APP operation

The instrument provides the Bluetooth wireless transmission function and a mobile phone APP, through which the user can remotely view measurement data. The App supports Android operating system 5.0 and above. You can use your mobile browser or WeChat to scan the QR code on the cover page. Download and install it as prompted. For details on APP operation, please refer to the APP and software user manual in the attached U disk.

6. PC software operation

The instrument offers USB interface and the PC software. It provides multiple functions, such as reading of all the recorded data in the instrument on the PC software, displaying of the power curve, exporting of the power data to EXCEL, printing of the report, etc. For details, please refer to the PC software and its user manual in the attached U disk.

VI. Measurement and precautions

1. When not in use, please long press the  button to power off.
2. Avoid contacting with corrosive materials and keep away from high humidity.
3. After shutdown, store it in a special packing box and keep it in a safe place. Protect the photosensitive part of the probe from polluting.
4. The recommended period of calibration is one year.
5. Because the UV probe is sensitive to humidity changes, the environment in which it is stored is important. When not in use for a long time, be sure to store the instrument in a low humidity environment.
6. When the instrument displays low battery, replace the battery.

VII. China National Standard

- 1) WS/T 367-2012 "*Regulation of Disinfection Technique in Healthcare Settings*" Page 15, Appendix A.3 Effect monitoring of ultraviolet disinfection.
- 2) The 2009 version of "*Technical Specifications for Disinfection in Hospitals*" Page 9, 2.3 UV disinfection.
- 3) Ultraviolet germicidal lamp GB19258-2003 Page 4, rated value of ultraviolet radiation intensity.

The above three national standards stipulate the following:

1. The peak wavelength of the ultraviolet germicidal lamp (low-pressure mercury lamp) is 253.7nm, which has a germicidal function.

2. The radiation intensity of the new 30W straight tube ultraviolet lamp is greater than $100\mu\text{W}/\text{cm}^2$ as qualified.
3. The radiation intensity of the 30W straight tube ultraviolet lamp in use is greater than $70\mu\text{W}/\text{cm}^2$ as qualified.
4. Different powers and different shapes of ultraviolet lamps have different radiation intensity values that are judged to be qualified.
5. The UV probe is placed at the center of the tested ultraviolet lamp at a vertical distance of 1 meter.

VIII. UV scale hook

In order to comply with UV germicidal lamp national standards, the UV light meter must be located at a vertical one meter below the middle of a lamp tube to measurement. Our company also provides UV scale hooks, which is 1m long. Place the instrument as shown below and hang it directly onto the lamp to facilitate on-site measurement of UV intensity.




IX. Special instructions for germicidal lamp measurement

1. Determining whether UV lamp power is up to standard

In order to meet the requirements of disinfection regulations, the automatic shutdown time is not less than 5 minutes. It is recommended to set the automatic shutdown time to 10 minutes. The instrument can (1 to 10 minutes optional) automatically power off, data recorded before automatic shutdown.

- No.1 recorded data is the latest recorded data. The curve is drawn based on historical data stored every 1 second. P_{REC} is the power value of the last shutdown time, which is used to determine whether the germicidal lamp is qualified.
- The tester places the instrument in the manner required by the test standard, turns on the instrument, and turns on the germicidal lamp before leaving the site. After the disinfection is completed, turn off

the UV lamp (the disinfection time is generally much longer than 10 minutes, and the instrument has been automatically shut down at this time). The tester enters the site to turn on the instrument, and the data displayed on the instrument is the last measuring data.

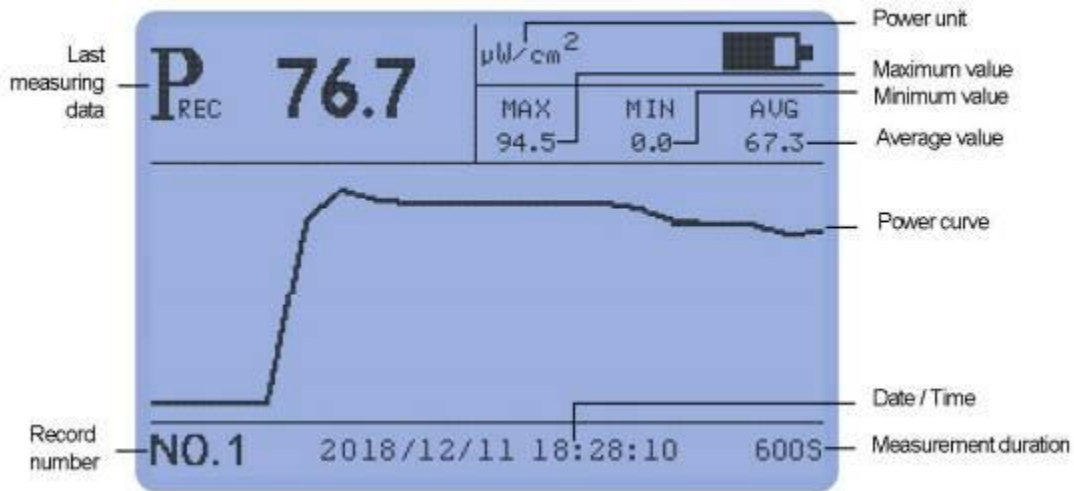

2. Monitor UV lamp power by APP via Bluetooth communication

The mobile APP is used to communicate with the instrument in real time. The data measured by the meter is sent to the mobile APP through Bluetooth, so that the user can monitor the power data of the UV lamp wirelessly. If the instrument automatically powers off during the measurement, the data of the mobile APP will not be updated. If it is necessary to continuously wirelessly monitor the instrument data with Bluetooth, the "Auto off" should be set OFF. At that time, the instrument is always as the active status and will not automatically shut down.

3. Data storage function

- When "Auto off" set ON, the data storage interval fixed to 1 second. The data storage time (Shutdown time) can be set from 1 to 10 minutes.
- The instrument can record up to 25 records. No.1 is the latest record. Record data without loss when power off.
- In the manual shutdown mode (Auto Off = OFF), the storage interval 1s/10s/60s correspond to the recording period 10 minutes/100 minutes/600 minutes, respectively. This facilitates to record the power value of the UV lamp for a long time.

X. Packing list

No.	Description	Quantity	Unit
1	UV Light Meter	1	pcs
2	USB cable	1	pcs
3	USB flash disk	1	pcs



4	AAA battery	4	pcs
5	UV scale hook	1	pcs
6	User manual	1	pcs
7	Calibration Report	1	pcs
8	Certificate/Warranty card	1	pcs
9	Plastic box	1	pcs

XI. Service

1. The meter has one-year warranty. If the instrument works abnormally, please send the whole instrument to our company for maintenance
2. Provide users with spare parts and lifelong maintenance services
3. Provide the users with the meter calibration service
4. Free technical support for long term

Manufacturer: Shenzhen Linshang Technology Co., Ltd.

Website: www.linshangtech.com

Service hotline: 086-755-86263411

Email: sales21@linshangtech.com